Forearm photo pair

ARTIFICIAL SAMPLE / **Digitally generated image pair**

Baseline **2 Mar 2026**

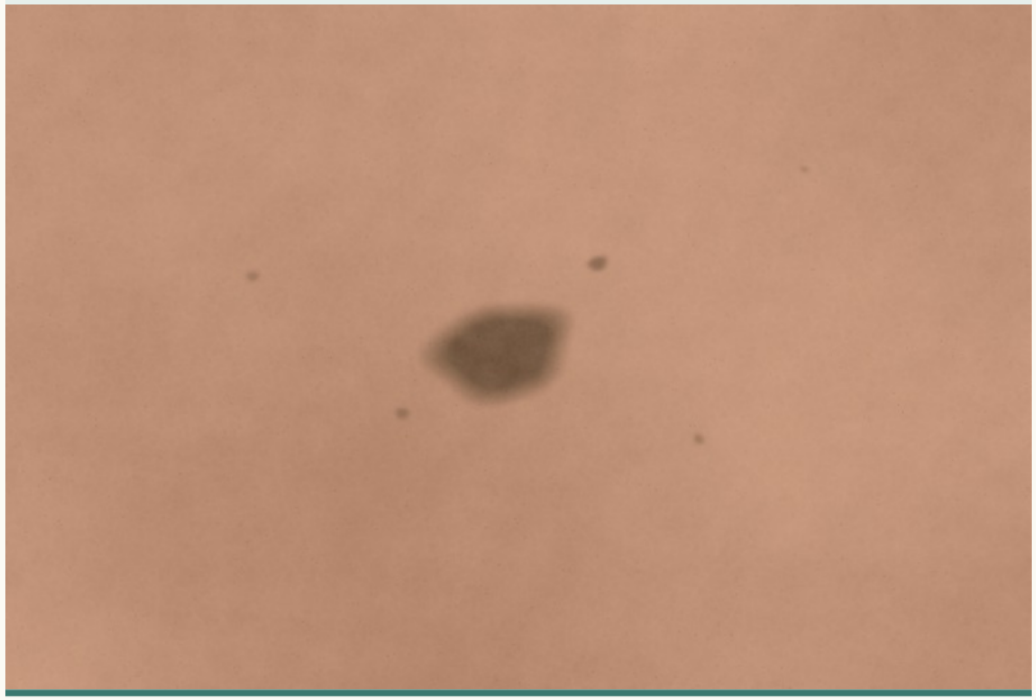

Follow-up **13 Apr 2026**

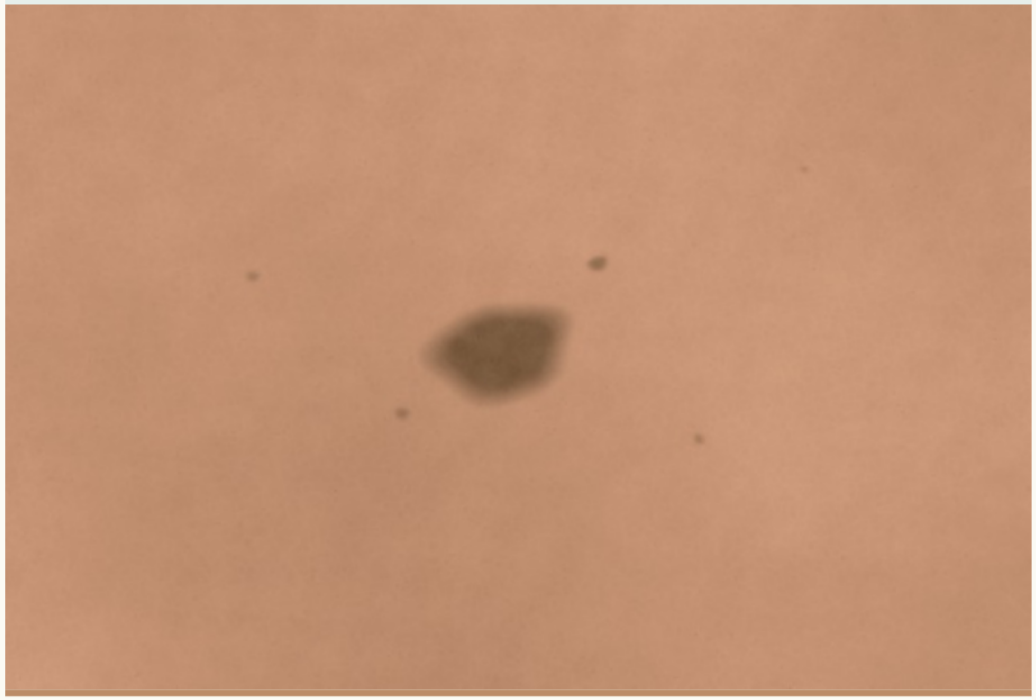

Patient notes

Artificial images of the same surface. The follow-up camera view was shifted and rotated, with warmer lighting. Use the small dot above and to the right of the central feature as an alignment landmark.

Follow-up alignment Zoom 115% · Rotation -4° · Horizontal -14 px · Vertical 9 px

Camera angle, distance and lighting affect appearance. Alignment does not establish physical scale or clinical change.